

DNA-coated AFM cantilevers for the investigation of cell adhesion and the patterning of live cells

Sonny C. Hsiao, Ailey K. Crow, Wilbur A. Lam, Carolyn R. Bertozzi, Daniel A. Fletcher and Matthew B. Francis*

The forces governing cell-cell adhesion are vitally important to many biological processes, including cell differentiation, tissue growth,^[1,2] tumorigenesis,^[1,3] and proper functioning of the

vertebrate immune response.^[4,5] The strengths of these interactions are typically characterized through the attachment of single living cells to probes that are capable of force measurement, such as suction micropipettes.^[6,7] More recently, optical tweezers^[8,9] have been applied to capture single cells and measure these forces with high accuracy, but this technique is limited to applying forces in the piconewton range.^[10] Atomic force microscopy (AFM)^[11] provides an attractive alternative to these methods because it is capable of quantifying forces in the piconewton to nanonewton range, and this technique has indeed been used to measure the mechanical properties of live single cells^[12] and study adhesion forces at the single cell level.^[13-19] Several fundamental adhesion measurements have been achieved by coating AFM cantilevers with fibronectin^[19] or lectins^[14,16,17,8] that bind to carbohydrate moieties on the cell surface, but especially in the latter case the cell binding molecules themselves have been reported to have a degree of cytotoxicity that can influence the cellular properties being evaluated.^[17,20,21,22] Thus, while these studies highlight the utility of AFM for the measurement of cell receptor-ligand interactions, an expanded set of cantilever attachment methods will be needed for the study of cell-cell interactions over widely varying time scales.

To address this need we have compared three biomolecule mediated methods for the attachment of live cells to AFM cantilevers, with an emphasis on the cell viability, adhesion strength, and probe reuse that each technique can achieve. These studies have indicated that cell attachment through the use of complementary DNA strands has the least influence on viability and does not appear to activate cell signaling pathways. This method also offers overall superior adhesion strength, but this parameter can be attenuated to allow cells to be transferred from one surface to another. We were able to demonstrate this concept by picking up free cells and placing them in exact positions on a substrate bearing DNA strands with longer complementary regions. This “Dip-Pen”^[23,24,25] live cell patterning demonstrates the reusability of the DNA-mediated cell adhesion method, and could prove useful for the construction of complex mixtures of cells with well-defined spatial relationships.

To allow the comparison of several attachment strategies, three different biomolecules (including DNA, concanavalin A, and an antibody) were attached to silicon nitride AFM cantilevers for cell anchoring. For all attachment methods, the thin layer of silicon oxide on the working surface was covered with aldehyde groups as outlined in Figure 1a. The surfaces produced using these steps were characterized by contact angle measurement

[*] S. C. Hsiao and Prof. M.B. Francis
Department of Chemistry
University of California, Berkeley
and
Materials Sciences Division
Lawrence Berkeley National Laboratory
Berkeley, CA 94720 USA
Fax: (+1) 510-643-3079
E-mail: francis@cchem.berkeley.edu

A. K. Crow
Biophysics Graduate Group
University of California, Berkeley

W. A. Lam
UCB/UCSF Joint Graduate Group in Bioengineering
University of California, Berkeley

Prof. D. A. Fletcher
Biophysics Graduate Group
University of California, Berkeley
and
UCB/UCSF Joint Graduate Group in Bioengineering
University of California, Berkeley

Prof. C. R. Bertozzi
Department of Chemistry & Molecular and Cell Biology
and
Howard Hughes Medical Institute
University of California, Berkeley
and
Materials Sciences Division
Lawrence Berkeley National Laboratory
Berkeley, CA 94720 USA

[**] We thank Z. Gartner, R. Chandra, E. Douglas, and X. Chen for technical assistance and helpful discussions, and especially Z. Gartner for DNA preparation. This work was supported by the Nanoscale Science, Engineering, and Technology (NSET) Program of the Department of Energy, and a National Research Service Award of National Institutes of Health and Hammond Research Fellowship of the National Childhood Cancer Foundation and Children's Oncology Group to W.A.L.



Supporting information for this article is available on the WWW under <http://www.angewandte.org> or the author.

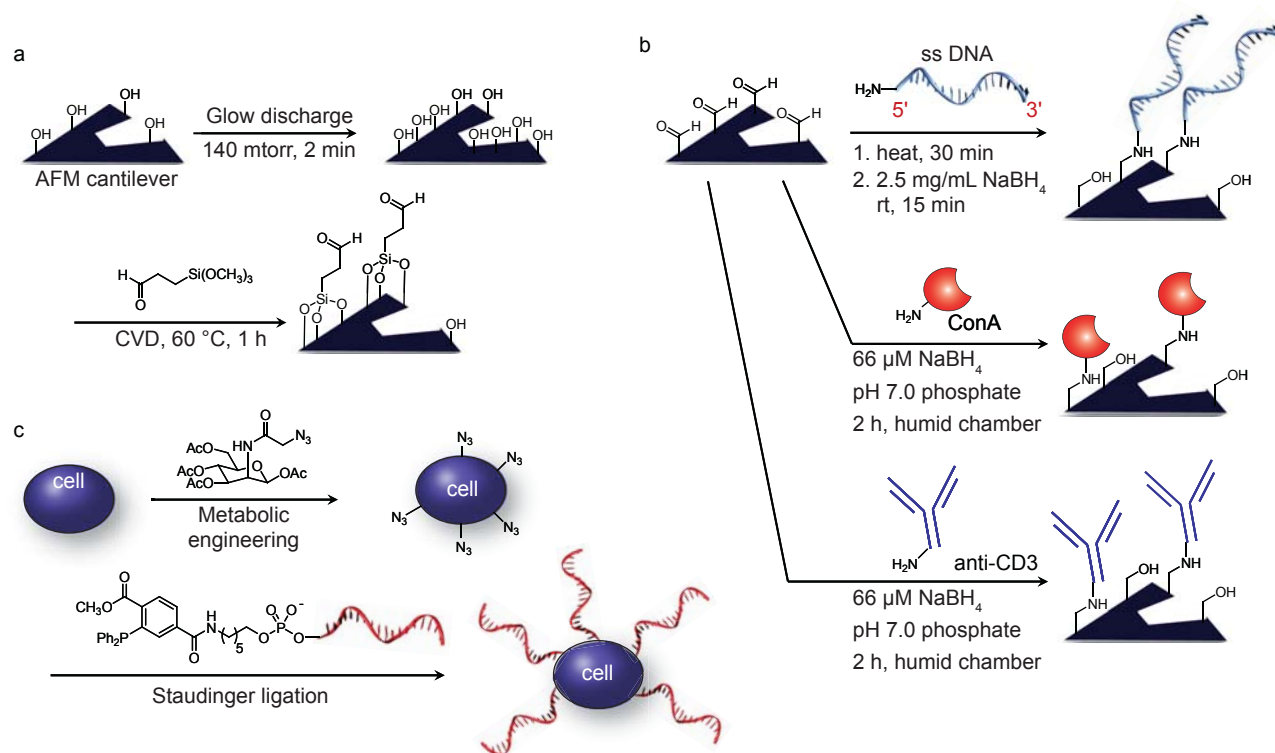


Figure 1. Covalent attachment of biomolecules to cantilevers and cell surfaces. **(a)** After surface oxidation using an oxygen plasma, aldehyde functional groups were introduced onto silicon nitride cantilevers using chemical vapor deposition (CVD). **(b)** Solutions of anti-CD3 IgG or ConA containing sodium borohydride were introduced onto aldehyde-coated cantilever surfaces in a humid chamber. DNA modification was achieved by immersing cantilevers in an amine functionalized ssDNA solution at 100 °C for 30 min, followed by exposure to a sodium borohydride solution. **(c)** Metabolic engineering was used to introduce azide groups onto cell surfaces via treatment with peracetylated-*N*-azidoacetylmannosamine (Ac_4ManNAz). Phosphine functionalized ssDNAs were synthesized and covalently attached to the exterior of cells via the Staudinger ligation.

(Supplementary Figure 1).

Amine functionalized DNA was attached to the aldehyde groups through reductive amination (Figure 1b).^[26,27] First, the aldehyde-coated cantilever was immersed in an amine functionalized single-strand DNA (ssDNA) solution and then heated to drive imine formation. After cooling to room temperature, an aqueous solution of sodium borohydride was used to reduce the imines to non-hydrolyzable amine linkages. This step also served to reduce any unreacted aldehyde functional groups to yield alcohols. By coupling 5'-amine functionalized DNA strands bearing fluorescein at the 3'-end, the presence of the strands could be verified by fluorescence imaging (Supplementary Figure 2).

In previous efforts, proteins have been attached to AFM tips through non-specific adsorption and through glutaraldehyde crosslinking to amine groups introduced on the tip surface.^[28] To afford more well-defined linkages (and thus realize more homogeneous cell attachment), we chose instead to use the simple reductive amination strategy that was used for the amino-DNA strands. Surface lysine residues on ConA and anti-human CD3 antibodies (anti-CD3) were reacted with the aldehyde functional groups on the cantilever surfaces (Figure 1b),^[29] but a lower concentration of reducing agent (66 μM) was used to minimize the reduction of disulfide bonds that are required to maintain protein tertiary structure.^[30,31,32] The concentrations of the

proteins (20 μM ConA and 6 μM anti-CD3) used in the reactions are easily achieved using commercially available samples. As described above for DNA, FITC-labeled ConA and anti-CD3 samples were used in some experiments to verify biomolecule attachment using fluorescence microscopy (Supplementary Figure 3). **Similar levels of fluorescence were detected for each.**

To prepare live cells bearing ssDNA on their surfaces, we first introduced azide functional groups into glycoproteins embedded in the plasma membrane, as previously described.^[33] Peracetylated *N*- α -azidoacetylmannosamine (Ac_4ManNAz) was added to cells, which then metabolized and displayed the azide on their surfaces (Figure 1c).^[34] Triarylphosphine-modified ssDNA was prepared through the reaction of 5'-amine-modified ssDNA with a phosphine pentafluorophenyl (PFP) ester. This reagent was then used to label the cell-surface azides through a Staudinger ligation,^[35] yielding stable amide linkages. Flow cytometry experiments have previously verified the ability of phosphine-DNA conjugates to undergo ligation to azide-modified cell surfaces.^[33] Although many cell types would be expected to be compatible with this system (and have been explored previously using the DNA-based adhesion method),^[33] non-adherent Jurkat cells were chosen for these studies because they do not secrete their own extracellular matrix. Thus, all cell adhesion events arise solely from the biomolecules on their surfaces.

The effects of the adhesion molecules on the viability of

the cells were assessed using two different methods. First, suspensions of unmodified Jurkat cells were supplemented with ConA or anti-CD3 antibodies, and the solutions of DNA-coated cells were supplemented with the complementary sequence. Figure 2a shows the growth curves of the resulting cells over a three day period. The propagation of the DNA modified cells was the same as that of unmodified cells, but the anti-CD3 treated cells showed delayed growth. ConA coated cells aggregated and were no longer alive after 12 hours. The morphologies of the cells after the addition of the reagents are shown in Supplementary Figure 5.

As a second comparison method, the three cell adhesion molecules were coated onto commercially available aldehyde-coated glass slides using the same reductive amination procedures outlined above. By visual inspection, all of three surfaces were able to achieve efficient cell binding (Figure 2b), but only the DNA-conjugated cells appeared morphologically unchanged after 48 hours. The ConA- and anti-CD3-immobilized cells exhibited significant changes during this time period, likely due to crosslinking of their surface receptors.^[36,37,38] The viability of the surface-immobilized cells was determined after 24 and 48 h using annexin V and propidium iodide (PI) staining.^[39] For the DNA-immobilized cells, the low percentage of apoptotic and necrotic cells was similar to that of unmodified cells (Figure 2c). However, the ConA and anti-CD3 immobilized cells showed significantly higher numbers of apoptotic cells compared to the control samples. Thus, the DNA molecules appear only to hybridize with their complementary partners, and should have much less potential to disturb the overall physiology of the cells in force measurement experiments.

Live cells were readily captured by AFM tips bearing all three of the biomolecules. This was accomplished simply by touching the cell membrane with the cantilevers, with contact times as short as 5 seconds resulting in the transfer of the cells to the AFM tips (see Supporting Information Movie 1). No cells were captured by tips lacking the appropriate biomolecules.

Our assay to determine the strength of cantilever attachment was designed such that cell-cantilever adhesions were fewer in number, and therefore weaker overall, than DNA-based adhesions between a cell and the complementarily functionalized glass slide. Due to this arrangement the cell-cantilever interaction would be expected to rupture first, yielding the strength of the interaction that a relatively low concentration of biomolecules can achieve. Rupture of the cell-cantilever interaction before the cell-surface interaction was verified by visual observation during experiments. The force of de-adhesion was measured for each attachment method using two different retraction rates and two different contact forces (Figure 3a). The measured force of de-adhesion increased with contact force and retraction rate across all attachment methods, as predicted by the Bell model.^[40] The ConA attachment method yielded zero-force attachment events in 12% of the de-adhesion measurements. Such events were not observed in the DNA and antibody cases.

A significant spread of forces was observed for all three attachment methods; however under all experimental parameters, the DNA method displayed the strongest average adhesion, followed by antibody attachment, then ConA (Figure 3b). As a

control experiment, we have also demonstrated that the capture efficiency of ConA and anti-CD3 is not affected by the presence of DNA strands introduced on the cell surface (Supplementary Figure 6). It should be noted that the overall de-adhesion forces determined for each attachment strategy depend on both the number of linkages and the retraction rates,^[40] and therefore do not reflect the absolute strengths of the individual biomolecular interactions. For the purpose of comparison, the force required to separate a typical 20 bp DNA duplex has been previously determined to be 38-50 pN,^[41] suggesting that in our experiments roughly 20-25 individual linkages are made between the cell and the cantilever. Similar reasoning would suggest that about 10 ConA-mannose interactions (at 47 pN each^[42]) and 12 antibody-antigen interactions (at 49 pN each^[43]) are involved, if the interaction strengths are assumed to be simply additive. Experiments to determine the number of linkages that are involved in each adhesion event are in progress in order to determine these effects more accurately. Nevertheless, our current results show that the DNA hybridization method leads to the most robust attachment under typical preparation conditions even though the strength of each individual linkage is likely to be less than that of the other biomolecules.

The strength of the cell-cantilever interaction can be tuned

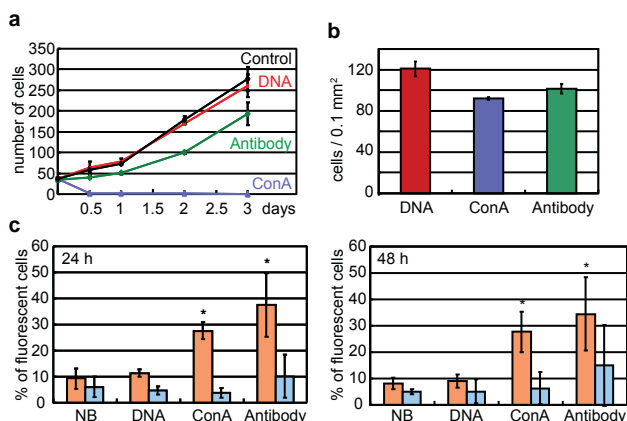


Figure 2. Comparison of biomolecule based adhesion methods. **(a)** Bulk cell growth rates were first determined in the presence of the adhesion molecules. A suspension of Jurkat cells was combined with ConA or anti-CD3 IgG, and a solution of DNA coated cells was combined with the complementary DNA strands. At various time points the total number of cells was counted. The control sample was grown in the absence of any adhesion molecules. **(b)** To evaluate cell capture efficiency, solutions of 20 μ M FITC-labeled ssDNA, 20 μ M FITC-labeled ConA, and 6 μ M FITC-labeled anti-CD3 IgG were applied to aldehyde-coated glass slides and the biomolecules were attached via reductive amination. Solutions containing 1×10^7 Jurkat cell/mL were then introduced onto the resulting slides. The samples were incubated for 10 min at room temperature, and then washed with two portions of PBS before evaluation. **(c)** To evaluate cell viability, cells were immobilized on DNA, ConA, and anti-CD3 IgG coated aldehyde slides. After immobilization for 24 h and 48 h, the cells were incubated with a solution of annexin V-FITC (orange bars) and PI (blue bars). The cells were evaluated within 1 h by fluorescence microscopy. *ConA and antibody immobilized cells that were partially stained by annexin were counted as cells undergoing apoptosis. NB represents control samples that were not bound to the surfaces.




Figure 3. AFM measurement of de-adhesion force. **(a)** Six sample traces for a single cell are shown in lighter colors, with the average trace shown in black. At zero distance, the cell is in full contact with the cantilever that is applying a positive force. As distance increases, the cantilever is pulled away from the glass slide surface, causing the cell-cantilever linkage to rupture and result in the zero-force, no-contact region. The force of de-adhesion was calculated as the difference between the curve minimum and the horizontal no-contact region. **(b)** Adhesion forces were measured under different retraction rates (15.7 $\mu\text{m/s}$ and 8.2 $\mu\text{m/s}$) and contact forces (400 pN and 200 pN) for the DNA, ConA, and antibody systems. Data were obtained by measuring six de-adhesion events on more than four different cells.

by varying the number of interacting strands and the length of the complementary regions, and the reversibility of DNA hybridization also allows the tips to be used many times. Both of these advantages allowed us to use AFM tips to arrange cells one at a time into patterns. In a recent report,^[44] it was shown that individual DNA strands could be moved from one location to another on a printed substrate, allowing small molecule dyes to be printed in a similar fashion.

To do this, a 5 μM solution of a shorter DNA strand (13 bases) was applied to the cantilever and an 80 μM solution of a longer strand (20 bases) was coupled to the glass slide. DNA-coated Jurkat cells were incubated in CO_2 independent media and applied to the non-coated side of glass slide under an AFM. The cantilever was then lowered into contact with the cell for 10 seconds with a contact force of 400 pN. The cantilever was then retracted, and cell attachment to the cantilever was confirmed visually (Supplementary Movie 1). The attached cells were then moved to the DNA coated side with maximum rate of 1 mm/s. The cantilever was lowered into contact with the slide, and the cell was allowed to interact with the substrate for 10 s with a 400 pN contact force. The cantilever was then retracted, whereupon the cell remained attached to the glass slide. By applying this printing method, cells can be given an (x,y) coordinate to position them precisely on a 2D substrate (Figure 4). The cells were found to remain viable after patterning, as shown in Supplementary Figure 7.

In summary, we have described the development of a versatile DNA-based adhesion method for the study of cell-cell interactions by AFM. The key advantages of this platform include the reusability of the tip, the tunability of the interaction strength, and the use of well-defined chemical linkages. Of the three biomolecule-based attachment strategies that were used, the DNA method proved superior in terms of cell viability after attachment. The use of AFM to form accurate and programmable patterns of individual cells provides a useful tool that can be used to understand the influence of neighboring interactions




Figure 4. Dip-Pen patterning of live cells. **(a)** By attaching a shorter DNA strand (13 bases) to a cantilever and a longer strand (20 bases) to the glass slide, a single living cell can be transported by the AFM and directly printed at a desired location on the glass slide. This process is shown stepwise for the formation of a single pattern of cells in **b-d**.

on cell differentiation and regulation. In a previous report, we have shown that complex patterns can be prepared through the self-assembly of DNA-coated cells on surfaces printed with complementary oligonucleotides.^[45] The AFM dip-pen method described here provides a useful complement to this technique that can achieve the higher resolution that would be needed to create and interrogate clusters consisting of multiple cell types. We are currently using this method to elucidate fundamental adhesion mechanisms involved in cancer metastasis, immune synapse formation, and cell-cell communication.

Received: ((will be filled in by the editorial staff))

Published online on ((will be filled in by the editorial staff))

This work was supported by the U.S. Department of Energy under Contract No. DE-AC02-05CH11231.

Keywords: AFM · DNA · Mammalian Cell · Patterning · Metabolic Engineering

- [1] D. E. Discher, P. Janmey, Y. L. Wang, *Science* **2005**, *310*, 1139.
- [2] M. Krieg, Y. Arboleda-Estudillo, P. H. Puech, J. Kafer, F. Graner, D. J. Muller, C. P. Heisenberg, *Nature Cell Biology* **2008**, *10*, 429.
- [3] M. J. Paszek, V. M. Weaver, *Journal of Mammary Gland Biology and Neoplasia* **2004**, *9*, 325.
- [4] S. I. Simon, C. E. Green, *Annual Review of Biomedical Engineering* **2005**, *7*, 151.
- [5] Y. van Kooyk, C. G. Figdor, *Current Opinion in Cell Biology* **2000**, *12*, 542.
- [6] J. Y. Shao, R. M. Hochmuth, *Biophysical Journal* **1996**, *71*, 2892.
- [7] Y. S. Chu, W. A. Thomas, O. Eder, F. Pincet, E. Perez, J. P. Thiery, S. Dufour, *Journal of Cell Biology* **2004**, *167*, 1183.
- [8] E. R. Dufresne, D. G. Grier, *Review of Scientific Instruments* **1998**, *69*, 1974.
- [9] O. Thoumine, P. Kocian, A. Kottelat, J. J. Meister, *European Biophysics Journal with Biophysics Letters* **2000**, *29*, 398.
- [10] H. Clausen-Schaumann, M. Seitz, R. Krautbauer, H. E. Gaub, *Current Opinion in Chemical Biology* **2000**, *4*, 524.
- [11] G. Binnig, C. F. Quate, C. Gerber, *Physical Review Letters* **1986**, *56*, 930.
- [12] M. Radmacher, in *Atomic Force Microscopy in Cell Biology*, Vol.


- 68, **2002**, pp. 67.
- [13] X. H. Zhang, E. Wojcikiewicz, V. T. Moy, *Biophysical Journal* **2002**, 83, 2270.
- [14] X. H. Zhang, E. P. Wojcikiewicz, V. T. Moy, *Experimental Biology and Medicine* **2006**, 231, 1306.
- [15] P. H. Puech, K. Poole, D. Knebel, D. J. Muller, *Ultramicroscopy* **2006**, 106, 637.
- [16] X. H. Zhang, A. Chen, D. De Leon, H. Li, E. Noiri, V. T. Moy, M. S. Goligorsky, *American Journal of Physiology-Heart and Circulatory Physiology* **2004**, 286, H359.
- [17] C. M. Franz, A. Taubenberger, P. Puech, D. J. Muller, *Science STKE* **2007**, 2007, 15.
- [18] M. Benoit, D. Gabriel, G. Gerisch, H. E. Gaub, *Nature Cell Biology* **2000**, 2, 313.
- [19] Y. Bustanji, C. Renata Arciola, M. Conti, E. Mandello, L. Montanaro, and B. Samori, *Proc. Natl. Acad. Sci. USA* **2003**, 100, 13292.
- [20] H. Ohba, R. Bakalova, M. Muraki, *Biochimica Et Biophysica Acta-General Subjects* **2003**, 1619, 144.
- [21] R. Ballerstadt, C. Evans, R. McNichols, A. Gowda, *Biosensors & Bioelectronics* **2006**, 22, 275.
- [22] R. Palacios, *Journal of Immunology* **1982**, 128, 337.
- [23] R. D. Piner, J. Zhu, F. Xu, S. Hong, C. A. Mirkin, *Science*, **1999**, 283, 661.
- [24] L. M. Demers, D. S. Ginger, S.-J. Park, Z. Li, S.-W. Chung, C. A. Mirkin, *Science* **2002**, 296, 1836.
- [25] D. S. Ginger, H. Zhang, and C. A. Mirkin, *Angewandte Chemie-International Edition*, **2004**, 43, 30.
- [26] M. Schena, D. Shalon, R. W. Davis, P. O. Brown, *Science* **1995**, 270, 467.
- [27] N. Zammattéo, L. Jeanmart, S. Hamels, S. Courtois, P. Louette, L. Hevesi, J. Remacle, *Analytical Biochemistry* **2000**, 280, 143.
- [28] M. D. Piramowicz, P. Czuba, M. Targosz, K. Burda, M. Szymonski, *Acta Biochimica Polonica* **2006**, 53, 93.
- [29] G. F. Zheng, F. Patolsky, Y. Cui, W. U. Wang, C. M. Lieber, *Nature Biotechnology* **2005**, 23, 1294.
- [30] P. Larsson, K. Mosbach, A. Borchert, US Patent 4532232, 1985.
- [31] M. Nisnevitch, M. A. Firer, *Journal of Biochemical and Biophysical Methods* **2001**, 49, 467.
- [32] M. Nisnevitch, M. Kolog-Gulco, D. Trombka, B. S. Green, M. A. Firer, *Journal of Chromatography B-Analytical Technologies in the Biomedical and Life Sciences* **2000**, 738, 217.
- [33] R. A. Chandra, E. S. Douglas, R. A. Mathies, C. R. Bertozzi, M. B. Francis, *Angewandte Chemie-International Edition* **2006**, 45, 896.
- [34] D. H. Dube, C. R. Bertozzi, *Current Opinion in Chemical Biology* **2003**, 7, 616.
- [35] E. Saxon, C. R. Bertozzi, *Science* **2000**, 287, 2007.
- [36] R. P. Macdermott, G. S. Nash, M. J. Bertovich, N. S. Merkel, I. J. Weinrieb, *Cellular Immunology* **1978**, 38, 198.
- [37] A. Freywald, N. Sharfe, C. D. Miller, C. Rashotte, C. M. Roifman, *Journal of Immunology* **2006**, 176, 4066.
- [38] J. H. Phillips, L. L. Lanier, *Journal of Immunology* **1986**, 136, 1579.
- [39] X. Chen, A. Kis, A. Zettl, C. R. Bertozzi, *Proceedings of the National Academy of Sciences of the United States of America* **2007**, 104, 8218.
- [40] G. I. Bell, *Science* **1978**, 200, 618.
- [41] T. Strunz, K. Oroszlan, R. Schäfer, H.-J. Güntherodt, *Proc. Natl. Acad. Sci. USA*, **1999**, 96, 11277.
- [42] T. V. Ratto, K. C. Langry, R. E. Rudd, R. L. Balhorn, M. J. Allen, M. W. McElfresh, *Biophys Journal*, **2004**, 86, 2430.
- [43] S. Allen, X. Chen, J. Davies, M. C. Davies, A. C. Dawkes, J. C. Edwards, C. J. Roberts, J. Sefton, S. J. B. Tandler, P. M. Williams, *Biochemistry*, **1997**, 36, 7457-7463.
- [44] S. K. Kufer, E. M. Puchner, H. Gump, T. Liedl, H. E. Gaub, *Science* **2008**, 319, 594.
- [45] E. S. Douglas, R. A. Chandra, C. R. Bertozzi, R. A. Mathies, M. B. Francis, *Lab on a Chip* **2007**, 7, 1442.

Entry for the Table of Contents

{{catch phrase}}

Sonny C. Hsiao, Ailey K. Crow, Wilbur A. Lam, Carolyn R. Bertozzi, Daniel A. Fletcher and Matthew B. Francis

DNA-coated AFM cantilevers for the investigation of cell adhesion and the patterning of live cells



DISCLAIMER

This document was prepared as an account of work sponsored by the United States Government. While this document is believed to contain correct information, neither the United States Government nor any agency thereof, nor the Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or the Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or the Regents of the University of California.